





Labelling field

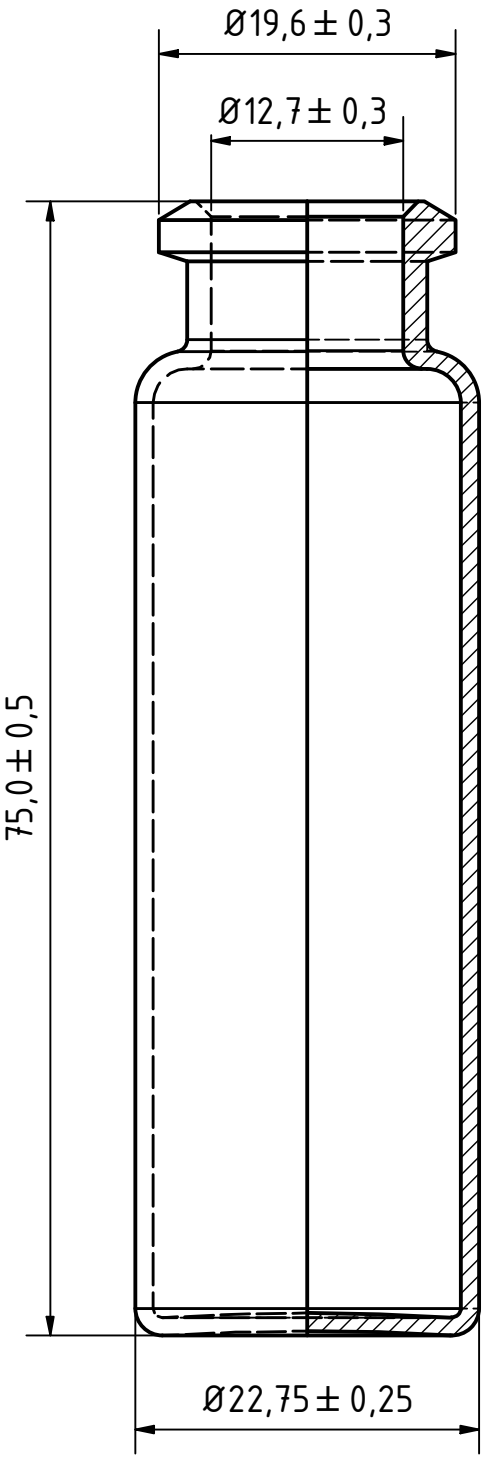



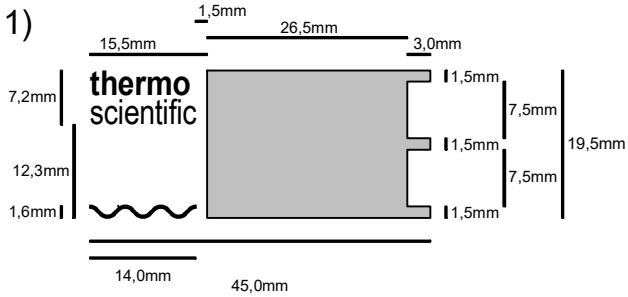

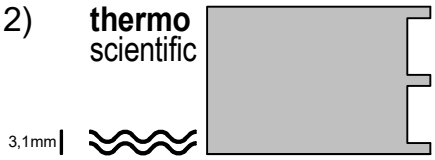

Part Number	Glass type / Borosilicate glass class	Labelling field 1 / 2 / 3
6PCV20-1F	Clear / 33	3

Bottom slanting must be less than 1.5°
*** Radial tolerances assigned as per DIN ISO 2768-1, unless otherwise specified**
Vials should be supplied free of visible contamination

Thermo Fisher SCIENTIFIC

Modification:	Name:	Date:	Approval Product Manager: pp. D.Lennartz	Date: 21.10.21	Drawn: Heich
			Approval QA:	Date: 14.02.2022	Date: 08.09.2021
			Part Number: 6PCV20-1F __ Customer		
Revision: 0	Date: 14.02.2022		Description: VIAL 20ML CLEAR CRIMP 20MM HEADSPACE BEVELD EDGE FLAT BOTTOM 22.75x75		page 1 of 1

All rights to this drawing are our property. This document contains confidential, proprietary information of Thermo Fisher Scientific. It may not be reproduced or copied without prior written permission from Thermo Fisher Scientific.