


DESCRIPTION

Logger-Trac™ RH/Temperature Datalogger is a multi-use, user programmable, humidity and temperature data recorder specifically designed for measuring environmental humidity and temperature during transportation of refrigerated vaccines, biological material, chemicals, pharmaceuticals, and for documenting transportation of perishable commodities.

Features

- RH Range: 0 to 100% RH
- Temperature Range: -29 to 72°C
- User programmable
- Small form factor
- Alarm and recording status LEDs
- IP66 Waterproof Rating
- USB interface

LCD DISPLAY

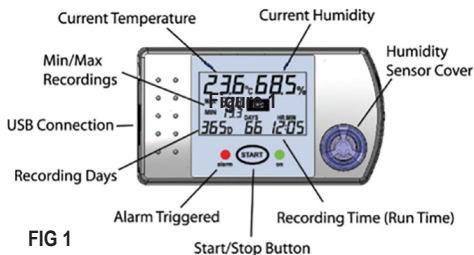

Current Temperature – The current temperature reading

Current Humidity – The current humidity reading

Min/Max Recordings – The minimum and maximum temperatures that have occurred since the device was initialized.

Start/Stop button – The button is used to start the device logging once it has been initialized. Hold button down for 3 seconds to activate logging. If the Stop key feature is enabled, pressing and holding the button will stop logging preemptively. Note: if the thermometer is stopped using the Stop button, the thermometer must be reinitialized using the MaxiThermal software before logging may be restarted.

Alarm Triggered – Indicates the temperature is in an active alarm state.

Recording Time (Run Time) – Indicates the amount of time passed since the thermometer logging was initialized/started.

PROGRAMMABLE USER SETTINGS

Through MaxiThermal software and USB interface, the user is able to program the unit to their specific requirements. Programmable options are listed as follows:

- **Description** – Each Logger-Trac device may be programmed with a unique description. This allows the user to identify at the time of download where the device was used.
- **Time zone**

- **Auto Adjust Daylight Time enable** – The internal clock will automatically adjust when daylight savings time shift occurs.

- **Temperature Measurement Units (Celsius/Fahrenheit)** – The temperature data will display on the LCD in the selected measurement units.

- **Start delay** – When this feature is used, a time delay occurs before data recording is started after the user presses the START button.

- **Recording duration/Sample Interval** – The user can either select the data recording interval or the total recording duration. Note the parameters are dependent upon each other so changing one field also changes the other.

- **Alarm setting** – Maximum and minimum alarm temperature boundaries can be set. The setting resolution is 1°.

- **No alarm** – Disable the alarm with this option.

- **User Stop Key Enable** – This feature allows the user to halt data recording by holding down the START button on the device once recording is started.

PRE-PROGRAMMED SETTING

All units are pre-programmed at factory with the following settings:

- Temperature Units: Celsius
- Alarm setting – Minimum: 2°C Maximum: 8°C

- Recording Duration: 30 days
- User Stop Key Enable: enabled

HOW TO START THE DATA LOGGER

1. Initialize Logger-Trac using MaxiThermal software to desired settings.
2. Disconnect thermometer from USB cradle.
3. When ready to begin recording, press and hold the START button for 3 seconds on the front panel. The LCD will become active and display the current temperature as well as the REC symbol to indicate logging is now active.
4. Place thermometer in environment to begin monitoring.

HOW TO STOP THE DATA LOGGER

1. The logging can be stopped in advance of the preprogrammed logging duration time by plugging the thermometer into the USB cradle and selecting Stop under the Logger Menu in MaxiThermal software. Also, if the stop key feature is enabled, the user may stop the thermometer logging by pressing and holding the START button for 3 seconds. The LCD will display the word END once logging is stopped.
2. Once the device has been stopped, the user may download the logged data from the thermometer.
3. Logging cannot be restarted until the thermometer has been reinitialized using MaxiThermal.

HOW TO REPLACE BATTERY

On back the Data Logger, turn the round plate counterclockwise, and replace with a new CR2016 3V Lithium Coin Cell battery. Turn the plate clockwise to lock.

Technical service

Web Resources

Visit the VWR's website at www.vwr.com for:

- Français, Español, Deutsch, Italiano, Português version
- Complete technical service contact information
- Access to VWR's Online Catalogue, and information about accessories and related products
- Additional product information and special offers

Contact us for information or technical assistance contact your local VWR representative or visit. www.vwr.com.

Warranty

VWR International warrants that this product will be free from defects in material and workmanship for a period of two (2) years from date of purchase. If a defect is present, VWR will, at its option, repair, replace, or refund the purchase price of this product at no charge to you, provided it is returned during the warranty period. This warranty does not apply if the product has been damaged by accident, abuse, misuse, or misapplication, or from ordinary wear and tear. For your protection, items being returned must be insured against possible damage or loss. This warranty shall be limited to the replacement of defective products. IT IS EXPRESSLY AGREED THAT THIS WARRANTY WILL BE IN LIEU OF ALL WARRANTIES OF FITNESS AND IN LIEU OF THE WARRANTY OF MERCHANTABILITY.

**GO TO VWR.COM FOR THE LATEST NEWS,
SPECIAL OFFERS AND DETAILS OF YOUR LOCAL
VWR DISTRIBUTOR**

Cat. No. 10154-376 / 620-2326

©2015 92-6550-60 Rev. 1 011115



TRACEABLE[®] LOGGER-TRAC[™] RH/TEMPERATURE DATALOGGER INSTRUCTIONS