

Test Chromatogram



COLUMN DETAILS:

Catalogue Number: ACE-111-1546

Serial Number: A262689

Packing: ACE 3 C18

Length: 15cm

Batch: DV19-3511

Internal Diameter: 4.6mm

EVALUATION CONDITIONS:

Mobile Phase: MeOH:H₂O (80:20)

Flow Rate: 1.0 ml/min


Pressure: 3950psi

Storage Solvent:

Wavelength: 254nm

Temperature: 22°C

Mobile Phase

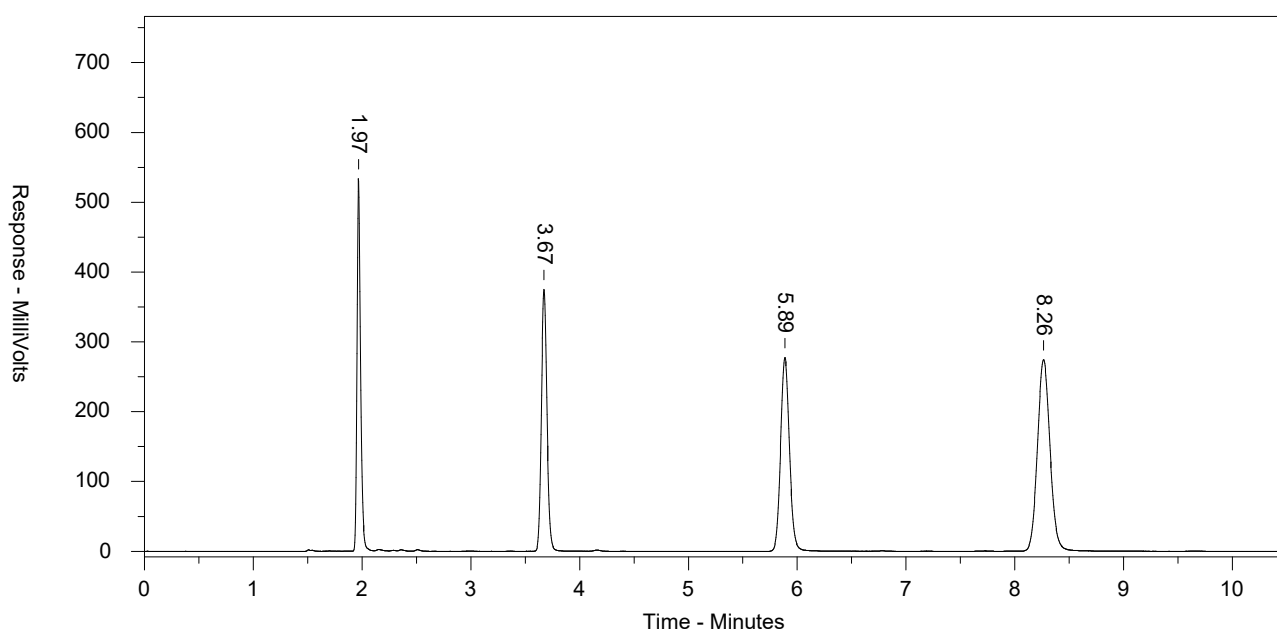

TEST RESULTS:

			Efficiency	Asymmetry Calculations		
Peak	Identity	t _r (minutes)	N _{0.5}	%	As _{0.1}	USP Tailing Factor
1	Dimethyl Phthalate	1.97	18000	84	1.60	1.35
2	Toluene	3.67	25100	93	1.20	1.13
3	Biphenyl	5.89	25700	94	1.15	1.10
4	Phenanthrene	8.26	24900	95	1.14	1.09

Care and Use of ACE[®] HPLC Columns

Thank you for purchasing this ACE[®] HPLC column.

Every ACE[®] HPLC column is manufactured and tested to exceed stringent specifications. The following measures will enhance its performance and lifetime.

Column Installation

System Dead Volume: Reduce dead volume in the system to a minimum by using connection tubing with an internal diameter of 0.010" (0.25mm) or less for analytical columns. Connections between injector, column and detector should be kept as short as possible.

Column Connection: The direction of flow is marked on the column. For optimum performance, the tubing connecting the column to injector and detector must abut the internal shoulder of the fitting. For HPLC columns, the use of PEEK fingertight fittings (p/n# ACE-FT10, 10 pack) are recommended.


Mechanical Damage: Protect the column from mechanical shock. Dropping a column can impair its performance.

Equilibration: This ACE HPLC column is shipped in the storage solvent defined overleaf on the test chromatogram. Flush onto the desired mobile phase (ensure that precipitation does not occur). Ensure that the column is fully equilibrated with the mobile phase prior to starting analysis.

Guard Cartridges: The use of guard cartridges is recommended to prevent both inlet frit blockage and irreversible sample adsorption onto the top of the column. Guard cartridges are available for all ACE HPLC columns - for assistance identifying the correct guard cartridge for this column, please contact our Technical Support Department at info@ace-hplc.com.

Precolumn Filters: As an alternative to guard cartridges, precolumn filters may be used to protect the column inlet frit from blockage. Due to their ultra low dispersion design, column performance and retention remain unaffected. For 3.0 - 4.6mm id ACE HPLC columns the use of analytical precolumn filters (p/n# ACE-CS210, 10 pack) are recommended. For 2.1mm id ACE HPLC columns, the use of microbore precolumn filters (p/n# ACE-HP210, 10 pack) are recommended.

Performance Testing: It is recommended that the performance of columns is tested on arrival and periodically during use. Performance parameters are defined below.

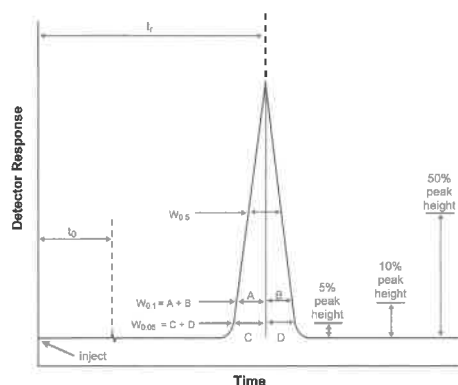

Performance

At 50% peak height

$$N_{0.5} = 5.54 (t_r / W_{0.5})^2$$

At 10% peak height

$$N_{0.1} = 18.55 (t_r / W_{0.1})^2$$

Peak Shape

Overlap to a perfect Gaussian peak

$$\% = N_{0.1} / N_{0.5}$$

Peak asymmetry
(measured at 10% peak height)

$$As_{0.1} = B/A$$

US Pharmacopeia Tailing Factor
(measured at 5% peak height)

$$T = W_{0.05}/2C$$

Selectivity

Retention factor

$$k = (t_r - t_0) / t_0$$

Operational Guidelines

Solvents: Use only HPLC grade solvents and freshly prepared aqueous buffer solutions to minimise bacterial growth. A slip-on pump inlet filter will remove extraneous particles. For maximum column lifetime, filter the mobile phase using a 0.2µm filter.

Mobile Phase pH: To ensure maximum column lifetime, a pH range of 2.0 - 8.0 is recommended. When operating at high pH, the use of an organic buffer is recommended. ACE SuperC18 columns provide an increased pH operating range of 1.5 - 11.5. For further information and guidance on maximising column lifetime under your chosen evaluation conditions, please contact our Technical Support Department at info@ace-hplc.com.

Sample: For maximum column lifetime, always use freshly prepared sample and filter using a 0.2µm filter.

Vials: For improved reproducibility and greater sample recovery of low abundance analytes, surface deactivated vials which virtually eliminate secondary interactions between sample and vial wall are recommended. Please contact our Technical Support Department at info@ace-hplc.com for further information.

Pressure: Exposure to rapid changes in pressure or pressures >4000psi (275bar) may reduce column lifetime.

UHPLC Column Availability: If a higher pressure rating is required, most ACE phases are additionally available in a dual compatible UHPLC/HPLC "Excel" hardware format with a 1000bar/15000psi pressure limit. Please contact our Technical Support Department at info@ace-hplc.com for further information.

Temperature: Exposure to temperatures >60°C may reduce column lifetime, dependent upon bonded phase and mobile phase conditions selected. For further guidance on maximising column lifetime under your chosen evaluation conditions, please contact our Technical Support Department at info@ace-hplc.com.

Storage: Wash out any buffer (ensure that precipitation does not occur) and flush onto the storage solvent defined overleaf. Replace the end-stops to prevent the packing bed drying out and store in a cool area.

Column Cleaning: Over a period of time, columns may still become contaminated by strongly adsorbed sample components. This may be indicated by a deterioration in column performance and/or an increase in back pressure. In such instances, specific cleaning protocols may be used in an attempt to regenerate column performance and further extend the lifetime of the column. For further guidance on the recommended cleaning protocol for this column, please contact our Technical Support Department at info@ace-hplc.com.

Column Warranty: All columns are warranted to meet the specifications stated on the Test Chromatogram. Removal of an end fitting to replace a frit or top-up the packing material should be regarded as a last resort to prolonging column lifetime. Removal of the column end fittings will automatically invalidate the column warranty.

Safety and Disposal: This column contains amorphous silica which may be hazardous to health if the column is unpacked and the silica allowed to dry. The silica presents no hazard whilst contained within the column. When the column has reached the end of its useful life, dispose of it in a similar manner to the samples that have been injected onto it. Alternatively, please contact our Technical Support Department at info@ace-hplc.com for details of our accredited column disposal program.

