

## STANDARD CONFIGURATION SUMMARY

- Chamber volume from 28 to 160 liters
- Working pressure meets ASME (USA) and PED (Europe) requirements
- Working at pressures of 0-325 kPa absolute
- Temperature range 60°C (140 F) to 138°C (280 F)
- Sterilization Temp. range 105°C (221 F) to 138°C (280°F)
- User friendly control system with multi-color display
- Up to 30 cycle programs (preset programs according to selected options)
- Stores the last 200 cycles in built-in memory of the controller
- USB and Ethernet communication ports
- Independent pressure gauge in front panel (not for 28xx model)
- 316L stainless steel chamber
- Two PT100 sensors
- Conforms to PED 97/23 EEC (Europe)
- Conforms to standards: ASME, UL (USA)
- Company Quality System Compliance with ISO 9001:2008 and ISO 13485:2003

## OPTIONAL FEATURES SUMMARY

- Fast Cooling by cooling coil (not for 2840 EL-D)
- Super-Fast cooling by fan and cooling coil (not for 2840 models)
- Vacuum pump for pre-vacuum air removal and post-vacuum moisture removal for improved drying, in combination with steam generators (EL models)
- F<sub>0</sub> calculation for sensitive loads
- Independent built-in steam generator
- Disinfection/Isothermal cycle 60°C (140°F) to 94°C (201°F)
- Warming Cycle 95°C (203°F) to 104°C (219°F)
- Biohazard system with a 0.2µm biological filter for decontaminating discharged air from the sterilizer
- Built-in printer
- External Independent Recorder
- User remote monitoring
- Advanced reporting system
- IQ, OQ, PQ
- Special Cycles for material testing

## PRODUCT DESCRIPTION

This autoclave series is designed to be highly customizable in order to cover a large range of applications for laboratories, research institutes and biotechnology facilities.

The autoclave series has a chamber volume range from 28 liters to 160 liters. The autoclave is heated by a heating plate on the outer chamber wall for Bench-top or heating element inside the chamber for Vertical. Optionally the autoclave can be equipped with a steam generator. All models have a temperature range from 60°C (140°F) to 138°C (280°F) and a working pressure that meets ASME (USA) and PED (Europe) requirements.

## APPLICATIONS

Laboratory  
Research Institutes  
Biotech Facilities  
Food laboratories  
Material Stress Testing  
Laboratory QA

Pharmaceutical Laboratory

## DEVICE PICTURE



2840EL-D Benchtop Autoclave



2840ELV-D Vertical Autoclave

Information provided by Tuttnauer is believed to be accurate and reliable. However, no responsibility is assumed by Tuttnauer for its use.

This specification is subject to change without notice.

# TECHNICAL SPECIFICATION – LABORATORY Autoclaves

## Benchtop and Vertical Series

### PRODUCT SPECIFICATION

#### CHAMBER VOLUME & SIZE

| MODEL                                                    | CHAMBER DIMENSIONS   |            | VOLUME (liters) |
|----------------------------------------------------------|----------------------|------------|-----------------|
|                                                          | Diameter $\phi$ (mm) | Depth (mm) |                 |
| 2840 EL-D<br>2840 ELC-G-D                                | 280                  | 400        | 28              |
| 2840 ELV-D<br>2840 ELVC-G-D                              | 280                  | 460        | 31              |
| 3850 EL-D<br>3850 ELC-G-D<br>3850 ELV-D<br>3850 ELVC-G-D | 380                  | 500        | 65              |
| 3870 EL-D<br>3870 ELC-G-D<br>3870 ELV-D<br>3870 ELVC-G-D | 380                  | 690        | 85              |
| 5050 EL-D<br>5050 ELC-G-D<br>5050 ELV-D<br>5050 ELVC-G-D | 500                  | 500        | 110             |
| 5075 EL-D<br>5075 ELC-G-D<br>5075 ELV-D<br>5075 ELVC-G-D | 500                  | 750        | 160             |

#### ELECTRICAL SAFETY AND COMPONENTS

All components are safety approved and certified by national and international organizations like UL, CE and others.

#### LANGUAGE

The operator display is available in the following 19 languages:

|         |            |
|---------|------------|
| English | Turkish    |
| German  | Czech      |
| Spanish | Romanian   |
| French  | Bulgarian  |
| Chinese | Hungarian  |
| Korean  | Vietnamese |
| Dutch   | Thai       |
| Russian | Danish     |
| Swedish | Serbian    |
| Polish  |            |

#### STANDARDS AND CODES

Our high quality laboratory autoclaves are designed to comply with the strictest international directives and standards.

#### Directives & Guidelines:

Pressure Equipment Directive – PED 97/23 EEC  
EMC Directive 89/336 EEC  
RoHS Directives – 2002/96 EEC  
Low Voltage Directive 73/23 EEC  
Machine Directive 2006/42

#### Standards:

DIN 58951-2:2003 Steam Sterilizers for Laboratory use  
ASME Code, Section VIII, Division 1, Unfired Pressure Vessels  
EN 13445:2009 for Pressure Vessels  
EN 14222:2003 for Stainless Steel Shell Boilers  
EN 13060 (only Annex C) - Water Quality

#### Safety and EMC Standards:

IEC/UL/EN 61010-1, IEC 61010-2-040, EN 61326

#### Good Practice Standards:

ISO 17665-1 and ST79

#### Quality System Compliance:

ISO 9001:2008 (Quality Systems)  
ISO 13485:2003 (Quality Systems for Medical Devices)

#### CHAMBER CONSTRUCTION

##### Materials

The sterilizer chamber is constructed from solid, high quality materials.

##### Chamber

Standard Chamber Material: Stainless Steel 316L  
Optional Chamber Material: Stainless Steel 316Ti

##### Design Pressure

Chamber is designed for 2.8 Bar(a)/142°C.

##### Door Gasket

A silicone gasket is permanently fixed in the door.

##### Surface Treatment

A passivation layer is applied to the internal surface through an electro-chemical treatment which results in a smooth and shiny stainless steel surface. The surface is polished to a Ra value < 0.8  $\mu\text{m}$  which is highly protective against corrosion.

#### CHAMBER HEATING

##### Standard

Benchtop autoclave: is heated by a heating plate on the outer chamber wall.

Vertical autoclave: is heated by an immersed heating element inside the chamber at the bottom.

##### Optional Advanced Heating (Steam Generator)

An integrated steam generator and a coiled pipe around the outer chamber wall can be used for heating benchtop or vertical autoclaves.

##### Insulation

The autoclave chamber is completely insulated with a chloride free glass wool thereby keeping the autoclave cool on the outside. The insulation reduces the energy consumption by keeping the heat inside the chamber.

#### SAFETY FEATURES

##### Door Safety Systems

The laboratory autoclaves are designed with a number of independent mechanical and electronic safety features.

## Benchtop and Vertical Series

- A safety device prevents the operator from opening the door when the chamber is pressurized
- Steam will not enter the chamber when the door is open
- A cycle cannot start if the door is open or not properly locked
- The controller will not allow the door to be unlocked until liquid temperature reaches the predetermined end temperature
- The controller will not allow the door to be opened until chamber pressure reaches room pressure

### General Safety Features

- **Safety Valves:** The chamber is equipped with safety valves – if the pressure exceeds the allowed limit the safety valves will discharge.
- **Built-in Steam Generator Safety:** A water level monitoring system maintains a constant water level and ensures safe operation of the heaters.

### VALVES

The piping system of the autoclave uses electrical solenoid valves to control the condensate and steam flow in and out of the chamber, to control the vacuum, and to control the air inlet valve.

### VALIDATION PORT

The chamber is provided with one threaded ¼" or ½" connection for optional vacuum/pressure gauges and test sensors.

### VACUUM PUMP (OPTION)

#### Prevacuum Air Removal & Post vacuum Moisture Removal

The optional vacuum pump effectively removes up to 99% air and moisture from the chamber. The pump is mounted on a shock absorber (damping mechanism) to minimize vibration. For model 2840 pre & post vacuum is achieved with a membrane pump.

### FAST LIQUID COOLING (OPTION)

**Importance of Cooling** - The chamber construction includes internal water coils (for benchtop autoclave) and external water coils (for vertical autoclave) which rapidly reduce the liquid temperature by the injection of cold water into these coils. This option is particularly useful for sterilizing sensitive liquid loads requiring reduced heat exposure time.

**Cooling Process** - Fast cooling is achieved by replacing steam with compressed air to equalize pressure and passing water through the cooling coils thereby reducing cooling time by as much as 75%. This results in safe cooling preventing breaking, deforming, damaging loads and reducing high temperature exposure time. Also, more sterilization cycles per day can be performed.

The installation site must include a separate compressed air utility to operate the cooling system.

### SUPER FAST LIQUID COOLING (OPTION)

In addition to fast cooling, an optional fan can be applied to further circulate the compressed air in the chamber. This speeds up the heat exchange during the cooling stage in order to safely achieve super-fast cooling of the liquid load under pressure. This can reduce cycle time up to 90% and minimizes load exposure to high temperatures

### Water and Air supply for all Fast Cooling Options

Water supply required for superfast cooling: 2 to 3 Bar pressure with a ½" diameter pipe.

Compresses air required for superfast cooling: 6 to 8 bar pressure with a ½" diameter pipe. 30 l/min. for 2840 models; 50 l/min. for models 3850 and up.

### VACUUM PUMP (OPTION)

#### Prevacuum Air Removal & Post vacuum Moisture Removal

The optional vacuum pump effectively removes up to 99% air and moisture from the chamber. The pump is mounted on a shock absorber (damping mechanism) to minimize vibration. For model 2840 pre & post vacuum is achieved with a membrane pump.

### DRYING OPTIONS

#### Active Drying with Post Vacuum

For benchtop autoclaves, an optional vacuum pump can be used for post vacuum drying, at the end of the sterilization cycle, ensuring improved drying of porous loads and hollow instruments such as pipette tips. The benchtop autoclave is equipped with a heating plate attached under the chamber that heats the chamber during the drying phase. The low pressure in the autoclave chamber, caused by the vacuum, reduces the boiling temperature forcing moisture to evaporate rapidly. The vapour is then removed from the chamber by vacuum resulting in a dry load.

#### Complete Drying with Chamber Heating and Post Vacuum

Highly efficient drying is achieved by uniformly heating the chamber wall of the benchtop or vertical autoclave. This is achieved by heating the chamber from steam passed through a coiled pipe around the chamber. The post vacuum stage reduces the boiling point which speeds up drying. This results in fast and complete drying, and guarantees that even the most difficult loads such as textiles, porous loads, hollow instruments and tips, will dry.

### PREVACUUM CYCLE (OPTION)

The prevacuum cycle is a fast and effective cycle for removing more than 99% of the air from the chamber in order to ensure good steam penetration and fast heating up.

### BIO-HAZARD SYSTEM (OPTION)

Tuttnauer's Bio-Hazard system provides an effluent sterilization cycle. Prior to sterilization, during the air removal stage, all effluent is passed through a 0.2µm biological filter that filters the exhaust air. During the sterilization phase, condensate does not leave the autoclave chamber where it is sterilized during the cycle together with the biological filter. After sterilization the sterilized effluent is cooled to a safe temperature before being discharged to drain.

### F<sub>0</sub> CALCULATION (OPTION)

F<sub>0</sub> calculation enables reduced media exposure to high temperatures thereby reducing cycle time and preventing damage to temperature sensitive media. Provisions are made to control the sterilization process by insertion of a temperature sensor (PT100) in the load. The exposure time measure is calculated using algorithm based software from the time the temperature sensor in the load has reached a predetermined set point until the end of the heat up stage. The F<sub>0</sub> value is recorded in the sterilization printout after the cycle completes.

### GRAVITY CYCLE

## Benchtop and Vertical Series

Non-porous goods, liquids and media in closed vented glass containers are suitable to be sterilized by a gravity cycle. The gravity cycle uses the gravity air displacement principle.

### DISINFECTION/ISOTHERMAL CYCLE (OPTION)

This cycle is designed to enable disinfection ("low" temperature isothermal treatment) typically used for preparing agar and other biological media. The temperature range setting is flexible within 60°C (140°F) to 94°C (201°F).

### WARMING CYCLE (OPTION)

The warming cycle has a temperature range from 95°C (203°F) to 104°C (219°F).

### TWO PT100 SENSORS

Two flexible PT100 temperature sensors inside the chamber are provided to monitor load temperature for sensitive liquid loads which require precise temperature and heat exposure control.

Safety is an important concern. Safety is ensured by using two PT100's to compare liquid temperatures between liquids in two vessels. If the temperature is different then it means a glass vessel may have broken.

Furthermore, two PT100s ensure glass vessels of different volumes in the chamber are sterilized and reach specified end temperature.

## STEAM SUPPLY OPTION

### Steam Generator

The optional independent built-in steam generator supplies steam for the sterilization process. The stainless steel steam generator is an electrically heated type generator equipped with immersion heaters.

The section "Electrical Specifications" provides detailed information about the electrical requirements for the autoclave when using an internal steam generator.

### Water Source for Steam Generator

Water to the steam generator is supplied by a single-phase pump which is connected to de-mineralized water source or RO water source.

### Steam Generator Water Quality

Various water systems can be used to supply mineral-free water to the steam generator such as Reverse Osmosis (RO), distilled water, etc. Water supplied to the steam generator should be in compliance with the EN 13060 (only Annex C) standard which includes the following hardness and conductivity requirements:

- Hardness ( $\Sigma$  Ions of alkaline earth) < 0.02 mmol/l
- Conductivity < 15  $\mu$ S/cm (at 20 °C)

**Note:** Soft water should not be used since its use may result in corrosion of the steam generator and chamber.

## VACUUM SYSTEM AND DRAIN COOLING WATER QUALITY

City tap water supply:

- Hardness between 0.7 and 2 mmol/l
- The tap water pressure should be in the range of 2 – 5 bar (30 - 72 psi)
- Recommended temperature: 15°C

## WATER CONSUMPTION OF MINERAL FREE WATER PER CYCLE

| Model | EL-D / ELC-D (Liters) | ELV-D / ELVC-D (Liters) |
|-------|-----------------------|-------------------------|
| 2840  | 0.8                   | 3                       |
| 3850  | 1.5                   | 8                       |
| 3870  | 2                     | 8                       |
| 5050  | 3                     | 20                      |
| 5075  | 5                     | 20                      |

## CONTROL SYSTEM

The main board controls and monitors the physical parameters of the sterilization process and performs the operation sequence of the machine, according to a user selected program, and includes the following features:

- F<sub>0</sub> software calculation (optional)
- PID (Proportional Integral Differential) pressure control
- Digital inputs and outputs for sterilizer control
- Analog inputs for control and reading temperature and pressure
- A USB port for external devices and an optional barcode feature. Direct connection to an internal thermal printer. An Ethernet communication port.
- Measures chamber pressure and steam generator pressure
- FLASH memory and real-time clock backup store cycle data for the last 100 cycles even if there is a power failure
- In/Out test
- Filter replacement notification based on number of cycles

The control system controls all system functions, monitors system operations, visually alerts the operator of cycle malfunctions and, on demand, provides visual indication of the chamber temperature and pressure.

## TEMPERATURE AND PRESSURE SENSORS

The temperature and pressure measuring circuits are both linear and designed with components having a high precision. The PT100 sensors conform to Class A of the IEC751 standard (ISO/EN 61010-2-040).

The control system allows for the calibration of temperature and pressure to be performed digitally.

Each sensor circuit is calibrated with individual constants to correct the deviation in manufacturing and aging.

## Benchtop and Vertical Series

The system uses FLASH memory in which the offset and gain data of the sensors are stored. This data may be entered into the system, through programming or through the autoclave control panel.

### CONTROL PANEL

#### Control and Monitoring

The control system is operated via the Bacsoft fully automated menu driven panel, consolidated into a 3 button circuit, allowing the user to easily operate, browse programs or set the autoclave

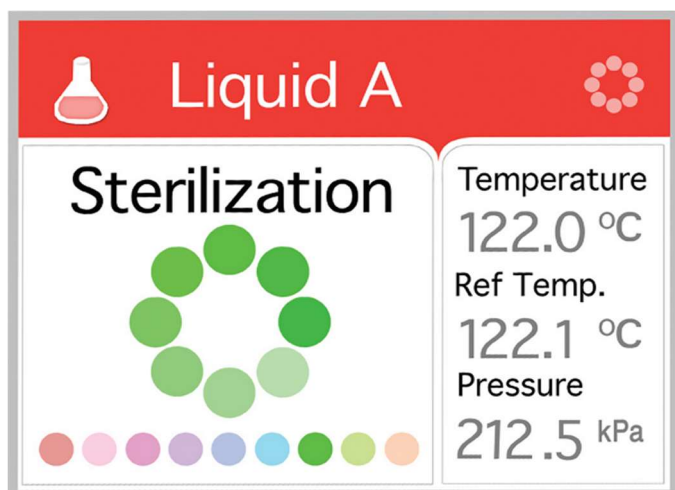
30 optional identification Codes and Passwords can be provided to control access/operation of the machine preventing unauthorized access. These access levels are customizable. Access control can be applied to functions, such as running test cycles, setting parameters, calibration, service and maintenance, cycle selection, cycle start and door control.

With the standard factory configuration, calibration of the temperature circuits and calibration of the pressure circuits require an access code.

### MULTI-COLOR DISPLAY

Human Machine Interface (HMI) has been designed with the following features:

- Color is used to indicate each stage of the cycle
- Quick access to important information
- Built-in view of historical cycle data
- Graphical display of temperature and pressure graphs
- Multiple languages



The following information is displayed:

- Temperature and pressure in the chamber
- Door status
- Sterilization time count down
- Autoclave status: standby, ready, pre-vacuum, heating, sterilization, exhaust, dry time, air inlet, cycle ended

### ALARMS AND INDICATORS

The autoclave uses audio alarms and visual indicators. Automatic process checking and failure detection are provided by the control system. In the event of a failure during the sterilization cycle, the system enters an alarm phase which will

safely end the process automatically. The range of alarms includes:

- Temperature & pressure sensor failure
- Phase time-outs
- Door(s) not properly closed
- Power failure
- No water in the water reservoir
- Optional utility alarms: no water / no steam / no air

### CYCLE DOCUMENTATION - PRINTER

The autoclave can be equipped with an optional printer which prints a detailed history of each cycle performed by the instrument. The printing format is 24 characters per line.

The following information is printed when the autoclave is turned on:

- Time & date when autoclave last turned off (powered down)
- Time & date when autoclave last turned on (powered up)

The following preliminary information and set parameters are printed when the sterilization cycle begins:

Cycle Start:

- Date
- Time
- Serial number
- Model name
- Software version
- Cycle number
- Cycle name

Sterilization Parameters

- Sterilization temperature
- Sterilization time
- End temperature
- Dry time (models with prevacuum and steam generator)

Thereafter, the autoclave starts performing the sequence of operations of the cycle. The measured values of temperature and pressure are printed at 1 minute time intervals. All interval times can be user defined. Furthermore, the customer may request customized time intervals prior to order delivery.

The data is printed beginning with the date and ending with "CYCLE ENDED" for a complete cycle or "CYCLE FAILED" for an aborted cycle.

## STERILIZER DOCUMENTATION

An Operation & Maintenance manual is provided, in English. The manual includes electrical and piping diagrams.

## MAINTENANCE / SERVICE PLAN

A global network of skilled service specialists can provide periodic inspections and adjustments to help assure low-cost peak performance. A detailed service and maintenance plan is included in the operator manual.

## PACKAGING FOR SHIPMENT

The sterilizer is packed in a wooden crate or rigid box for shipping/transportation.

## WARRANTY

Tuttnauer warrants that each device is carefully tested, inspected and that it leaves the factory in proper working condition.

Tuttnauer certifies that the device is guaranteed to be free from defects in material and workmanship, for one year from installation date but not more than 18 months from shipping date, against faulty components and assembly. Extended warranty periods are optional.

The warranty does not include and does not replace routine treatment and preventive maintenance to be performed according to "Preventive and Periodical Maintenance" instructions mentioned in the device's accompanying manual.

**The user must ensure that all utilities used, including the water, meet all the specifications mentioned in the operator manual.**

The user is subject to the full warranty statement found in the documentation delivered with the equipment.

## UTILITY DATA / REQUIREMENTS

### Drainage (Sewage)

1. At least 1/2" sewage pipe.
2. The sewage shall be able to withstand continuous temperature of 80 °C. The drain/sewage system should be able to withstand 120 °C in case of malfunction.

**Note:** Local national regulations may require that the drain be tapped and vented, and not connected to other drains which may cause back pressure or obstruct flow. An air break may also be necessary.

### Compressed Air (for fast cooling)

1. At least 1/2" hose to supply the compressed air
2. Compressed air pressure 6 – 8 Bar
3. Flow rate: 30l/min. for 2840 models; 50l/min. for 38xx and 50xx models
4. Building compressed air supply line requires shut-off valve
5. Pressure: 6 bar, free from liquid water droplets, filtered to 25 µm, free from oil droplets greater than 2 µm

### Ambient Temperature

Room temperature should be in the range from 5 to 40 °C and 85% RH (relative humidity).

### Mineral-Free Feed Water for Steam Generator

Water supplied to the steam generator should have the following hardness and conductivity requirements:

- Hardness ( $\sum$  Ions of alkaline earth) < 0.02 mmol/l
  - Conductivity < 15 µS/cm (at 20 °C)
1. Water intended for the steam generator must have a water quality in accordance with EN 13060 (only Annex C)
  2. Install 1/2" pipe with a shut-off valve at its end
  3. Regulations may require a Back-Flow protection device

**Note:** Soft water should not be used since its use may result in corrosion of the steam generator and chamber.

### Tap Water

1. Intended for vacuum pump and cooling
2. Install 1/2" pipe with shut-off valve at its end
3. Supply pressure 2 – 3 bar at approximately 15 °C temperature
4. Local regulations may require a Back-Flow protection device
5. Hardness (free of alkaline earth ions) should be between 0.7 mmol/l and 2.0 mmol/l

# TECHNICAL SPECIFICATION – LABORATORY Autoclaves

## Benchtop and Vertical Series

### ELECTRICAL SPECIFICATION

Models WITHOUT internal steam generator:

#### Front Loading EL Benchtop Models

| Model     | Voltage<br>V (50/60 Hz) | Phases | Power<br>(kW) |
|-----------|-------------------------|--------|---------------|
| 2840 EL-D | 208 / 230               | 1      | 2.2           |
| 3850 EL-D | 208 / 230               | 1      | 3.2           |
| 3870 EL-D | 208 / 230 / 380-400     | 3      | 4.8           |
| 5050 EL-D | 208 / 230 / 380-400     | 3      | 4.8           |
| 5075 EL-D | 208 / 230 / 380-400     | 3      | 6.6           |

#### Top Loading Floor Standing ELV Vertical Models

| Model      | Voltage<br>V (50/60 Hz) | Phases | Power<br>(kW) |
|------------|-------------------------|--------|---------------|
| 2840 ELV-D | 208 / 230               | 1      | 2.2           |
| 3850 ELV-D | 208 / 230 / 380-400     | 3      | 6             |
| 3870 ELV-D | 208 / 230 / 380-400     | 3      | 6             |
| 5050 ELV-D | 208 / 230 / 380-400     | 3      | 9             |
| 5075 ELV-D | 208 / 230 / 380-400     | 3      | 9             |

Models WITH internal steam generator:

#### Front Loading ELC-G-D Models

| Model        | Voltage<br>V (50/60 Hz) | Phases | Power<br>(kW) |
|--------------|-------------------------|--------|---------------|
| 2840 ELC-G-D | 208 / 230               | 1      | 2.2           |
| 3850 ELC-G-D | 208 / 230 / 380-400     | 3      | 9             |
| 3870 ELC-G-D | 208 / 230 / 380-400     | 3      | 9             |
| 5075 ELC-G-D | 208 / 230 / 380-400     | 3      | 9             |

#### Top Loading Floor Standing Vertical Models

| Model         | Voltage<br>V (50/60 Hz) | Phases | Power<br>(kW) |
|---------------|-------------------------|--------|---------------|
| 3850 ELVC-G-D | 208 / 230 / 380-400     | 3      | 9             |
| 3870 ELVC-G-D | 208 / 230 / 380-400     | 3      | 9             |
| 5050 ELVC-G-D | 208 / 230 / 380-400     | 3      | 9             |
| 5075 ELVC-G-D | 208 / 230 / 380-400     | 3      | 9             |

Models WITH water reservoir:

#### Top Loading Floor Standing Vertical Models

| Model         | Voltage<br>V (50/60 Hz) | Standard configuration<br>Phases | Power<br>(kW) | Optional configuration<br>Voltage V (50/60 Hz) | Optional configuration<br>Phases | Optional Power<br>(kW) |
|---------------|-------------------------|----------------------------------|---------------|------------------------------------------------|----------------------------------|------------------------|
| 2840 ELV-WR-D | 208 / 230               | 1                                | 2.2           | NA                                             | NA                               | —                      |
| 3850 ELV-WR-D | 208 / 230               | 1                                | 3.3           | 208 / 230 / 380-400                            | 3                                | 6                      |
| 3870 ELV-WR-D | 208 / 230               | 1                                | 3.3           | 208 / 230 / 380-400                            | 3                                | 6                      |
| 5075 ELV-WR-D | 208 / 230 / 380-400     | 3                                | 9             | NA                                             | NA                               | —                      |

Note: 3-phase autoclaves can be converted to 1-phase using a switch box (optional). Models 3850/70 ELV have a current consumption of 27A with a 1-phase connection. Models 5050/5075 have a current consumption of 40A with a 1-phase connection.

# TECHNICAL SPECIFICATION – LABORATORY Autoclaves

## Benchtop and Vertical Series

### EXTERNAL DIMENSIONS & WEIGHT

Models WITHOUT internal steam generator:

#### Front Loading EL Benchtop Models

#### Loading Floor Standing ELV Vertical Models

| Model     | External Dimensions<br>W x H x D (mm) | Weight (kg) |
|-----------|---------------------------------------|-------------|
| 2840 EL-D | 530 x 440 x 630                       | 43          |
| 3850 EL-D | 720 x 540 x 765                       | 120         |
| 3870 EL-D | 720 x 540 x 940                       | 130         |
| 5050 EL-D | 860 x 740 x 890                       | 203         |
| 5075 EL-D | 860 x 740 x 1120                      | 203         |

#### Top

| Model      | External Dimensions<br>W x H x D (mm) | Weight (kg) |
|------------|---------------------------------------|-------------|
| 2840 ELV-D | 540 x 980 x 440                       | 101         |
| 3850 ELV-D | 730 x 1000 x 540                      | 108         |
| 3870 ELV-D | 730 x 1000 x 540                      | 113         |
| 5050 ELV-D | 870 x 860 x 770                       | 215         |
| 5075 ELV-D | 870 x 1090 x 770                      | 215         |

Models WITH internal steam generator and fast cooling:

#### Front Loading ELC-G-D Models

| Model        | External Dimensions<br>W x H x D (mm) | Weight (kg) |
|--------------|---------------------------------------|-------------|
| 2840 ELC-G-D | 530 x 440 x 760                       | 50          |
| 3850 ELC-G-D | 730 x 1366 x 1190                     | 143         |
| 3870 ELC-G-D | 730 x 1366 x 1190                     | 153         |
| 5050 ELC-G-D | 870 x 1578 x 1175                     | 226         |
| 5075 ELC-G-D | 870 x 1578 x 1175                     | 226         |

#### Top Loading Floor Standing Vertical Models

| Model         | External Dimensions<br>W x H x D (mm) | Weight (kg) |
|---------------|---------------------------------------|-------------|
| 3850 ELVC-G-D | 730 x 1000 x 700                      | 124         |
| 3870 ELVC-G-D | 730 x 1000 x 700                      | 127         |
| 5050 ELVC-G-D | 870 x 1090 x 770                      | 224         |
| 5075 ELVC-G-D | 870 x 1090 x 770                      | 224         |

Models WITH water reservoir:

#### Top Loading Floor Standing Vertical Models

| Model         | External Dimensions<br>W x H x D (mm) | Weight (kg) |
|---------------|---------------------------------------|-------------|
| 2840 ELV-WR-D | 530 x 988 x 530                       | 68          |
| 3850 ELV-WR-D | 739 x 1075 x 800                      | 125         |
| 3870 ELV-WR-D | 739 x 1075 x 800                      | 131         |
| 5075 ELV-WR-D | 739 x 1075 x 800                      | 235         |

FLASK LOADING CAPACITY

**ERLENMEYER FLASKS**



| Vertical Models   | Erlenmeyer    |                  |        |        |        |        |
|-------------------|------------------------------------------------------------------------------------------------|------------------|--------|--------|--------|--------|
|                   | 250ml                                                                                          | 500ml            | 1000ml | 2000ml | 3000ml | 5000ml |
|                   | Quantity of Baskets X Quantity of Erlenmeyer flasks                                            |                  |        |        |        |        |
| 2840ELV / ELVC    | 2 x 5                                                                                          | 2 x 3            | 1 x 1  | 1 x 1  | 1 x 1  | 1 x 1  |
| 3850ELV / ELVC    | 2 x 12                                                                                         | 2 x 8            | 1 x 5  | 1 x 2  | 1 x 1  | 1 x 1  |
| 3870ELV / ELVC    | 3 x 12                                                                                         | 3 x 8            | 2 x 5  | 2 x 2  | 2 x 1  | 1 x 1  |
| 5050ELV / ELVC    | 2 x 21                                                                                         | 2 x 14           | 2 x 8  | 1 x 5  | 1 x 4  | 1 x 2  |
| 5075ELV / ELVC    | 3 x 21                                                                                         | 3 x 14           | 3 x 8  | 2 x 5  | 2 x 4  | 1 x 2  |
| Benchtop Models   | Erlenmeyer    |                  |        |        |        |        |
|                   | 250ml                                                                                          | 500ml            | 1000ml | 2000ml | 3000ml | 5000ml |
| Bottom shelf only |                                                                                                |                  |        |        |        |        |
| 2840EL            | 8                                                                                              | 4                | 2      | None   | None   | None   |
| 3850EL            | 18                                                                                             | 11               | 7      | 4      | 2      | None   |
| 3870EL            | 24                                                                                             | 14               | 10     | 5      | None   | None   |
| 5050EL            | 24                                                                                             | 15               | 11     | 6      | 4      | 2      |
| 5075EL            | 36                                                                                             | 24               | 15     | 8      | 7      | 3      |
| Benchtop Models   | Erlenmeyer  |                  |        |        |        |        |
|                   | 250ml                                                                                          | 500ml            | 1000ml | 2000ml | 3000ml | 5000ml |
| Shelves System    | * Optional Shelves System is not included in the Autoclave price                               |                  |        |        |        |        |
|                   | Quantity of Shelves X Quantity of Erlenmeyer flasks                                            |                  |        |        |        |        |
| 2840EL            | 1 x 9                                                                                          | 1 x 4            | 1 x 3  | None   | None   | None   |
| 3850EL            | 1 x 17                                                                                         | 1 x 11           | 1 x 6  | 1 x 3  | None   | None   |
| 3870EL            | 1 x 23                                                                                         | 1 x 17           | 1 x 10 | 1 x 5  | None   | None   |
| 5050EL            | 1 x 25<br>1 x 16                                                                               | 1 x 15<br>1 x 12 | 1 x 7  | 1 x 4  | 1 x 2  | 1 x 2  |
| 5075EL            | 1 x 50<br>1 x 18                                                                               | 1 x 18<br>1 x 18 | 1 x 15 | 1 x 7  | 1 x 4  | 1 x 3  |

### SCHOTT DURAN FLASKS

| Vertical Models   | Schott Duran  |                  |        |        |        |
|-------------------|-------------------------------------------------------------------------------------------------|------------------|--------|--------|--------|
|                   | 250ml                                                                                           | 500ml            | 1000ml | 2000ml | 5000ml |
|                   | Quantity of Baskets X Quantity of Schott Duran flasks                                           |                  |        |        |        |
| 2840ELV / ELVC    | 2 x 8                                                                                           | 2 x 5            | 1 x 3  | 1 X 1  | 1 X 1  |
| Benchtop Models   | Schott Duran  |                  |        |        |        |
|                   | 250ml                                                                                           | 500ml            | 1000ml | 2000ml | 5000ml |
| Bottom shelf only |                                                                                                 |                  |        |        |        |
| 2840EL            | 10                                                                                              | 8                | 4      | None   | None   |
| 3850ELV / ELVC    | 2 X 19                                                                                          | 2 X 12           | 1 X 8  | 1 X 4  | 1 X 1  |
| 3870ELV / ELVC    | 3 X 19                                                                                          | 3 X 12           | 2 X 8  | 2 X 4  | 1 X 1  |
| 5050ELV / ELVC    | 2 X 32                                                                                          | 2 X 21           | 2 X 15 | 1 X 8  | 1 X 4  |
| 5075ELV / ELVC    | 3 X 32                                                                                          | 3 X 21           | 3 X 15 | 2 X 8  | 2 X 4  |
| 3850EL            | 24                                                                                              | 17               | 12     | 7      | None   |
| 3870EL            | 33                                                                                              | 24               | 16     | 10     | None   |
| 5050EL            | 35                                                                                              | 24               | 15     | 8      | 4      |
| 5075EL            | 50                                                                                              | 36               | 24     | 13     | 8      |
| Benchtop Models   | Schott Duran  |                  |        |        |        |
|                   | 250ml                                                                                           | 500ml            | 1000ml | 2000ml | 5000ml |
| Shelves System    | * Optional Shelves System is not included in the Autoclave price                                |                  |        |        |        |
|                   | Quantity of Shelves X Quantity of Schott Duran flasks                                           |                  |        |        |        |
| 2840EL            | 1 x 12                                                                                          | 1 x 9            | 1 x 5  | None   | None   |
| 3850EL            | 1 x 27                                                                                          | 1 x 16           | 1 x 11 | 1 x 6  | None   |
| 3870EL            | 1 x 36                                                                                          | 1 x 23           | 1 x 18 | 1 x 9  | None   |
| 5050EL            | 1 x 35<br>1 x 27                                                                                | 1 x 20<br>1 x 16 | 1 x 12 | 1 x 6  | 1 x 3  |
| 5075EL            | 1 x 55<br>1 x 39                                                                                | 1 x 32<br>1 x 27 | 1 x 20 | 1 x 10 | 1 x 5  |

#### Loading configuration example:

Loading capacity 3850 ELV-D with 2 x 19 Scott Duran 250 ml bottles



**Benchtop and Vertical Series**

**CYCLE TIMES**

Note: Temperature measured in reference container

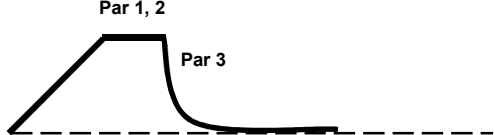
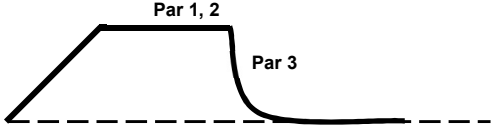
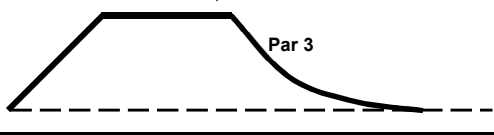
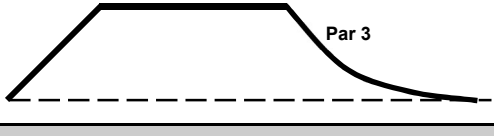
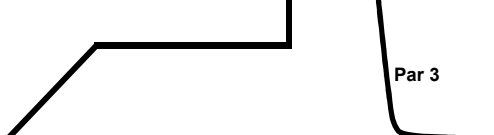
| Model                      | Loading Capacity | Heating Time<br>121 °C | Cooling Time<br>80°C without Cooling | Cooling Time<br>80°C with rapid cooling<br>and Radial Fan | Cooling Time<br>80°C with Rapid<br>Cooling |
|----------------------------|------------------|------------------------|--------------------------------------|-----------------------------------------------------------|--------------------------------------------|
| <b>Benchtop Autoclaves</b> |                  |                        |                                      |                                                           |                                            |
| 2840 EL                    | 1 x 250 ml       | 22 min                 | 52 min                               | -                                                         | 26 min                                     |
|                            | 8 x 500 ml       | 29 min                 | 138 min                              | -                                                         | 52 min                                     |
| 3850 EL                    | 1 x 500 ml       | 24 min                 | 72 min                               | 16 min                                                    | 29 min                                     |
|                            | 10 x 500 ml      | 30 min                 | 125 min                              | 25 min                                                    | 48 min                                     |
|                            | 8 x 2000 ml      | 47 min                 | 280 min                              | 61 min                                                    | 106 min                                    |
| 3870 EL                    | 10 x 1000 ml     | 42 min                 | 170 min                              | 37 min                                                    | 68 min                                     |
| 5050 EL                    | 20 x 1000 ml     | 44 min                 | 274 min                              | 46 min                                                    | 95 min                                     |
| 5075 EL                    | 15 x 2000 ml     | 50 min                 | 314 min                              | 73 min                                                    | 132 min                                    |
| <b>Vertical Autoclaves</b> |                  |                        |                                      |                                                           |                                            |
| 2840 ELV                   | 1 x 1000 ml      | 31 min                 | 87 min                               | -                                                         | 38 min                                     |
|                            | 10 x 500 ml      | 41 min                 | 161 min                              | -                                                         | 53 min                                     |
| 3850 ELV                   | 12 X 500 ml      | 25 min                 | 130 min                              | 24 min                                                    | 48 min                                     |
| 3870 ELV                   | 6 x 1000 ml      | 25 min                 | 151 min                              | 26 min                                                    | 50 min                                     |
|                            | 18 x 1000 ml     | 35 min                 | 270 min                              | 45 min                                                    | 95 min                                     |
| 5050 ELV                   | 6 x 2000 ml      | 33 min                 | 263 min                              | 51 min                                                    | 98 min                                     |
| 5075 ELV                   | 42 x 500 ml      | 44 min                 | 230 min                              | 48 min                                                    | 94 min                                     |

# TECHNICAL SPECIFICATION – LABORATORY Autoclaves

## Benchtop and Vertical Series

### PROGRAM CYCLE DATA

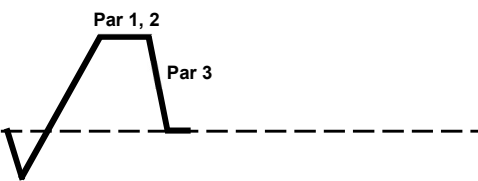
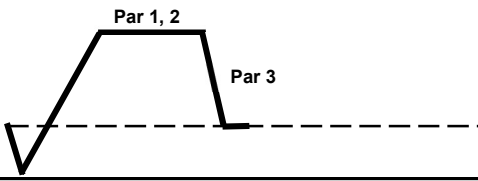
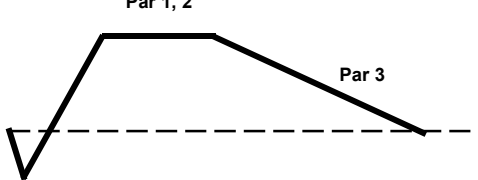
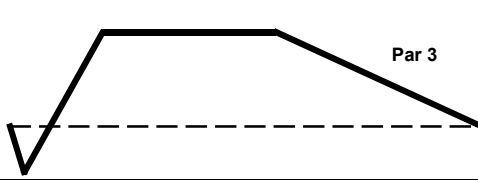
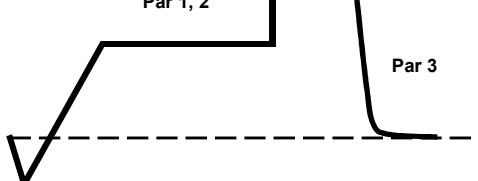
#### PROGRAMS 1 TO 6

| Program 1                                         |                                                                                     | Glass (Fast Exhaust)                                                                          |                           |                                                     |
|---------------------------------------------------|-------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------|---------------------------|-----------------------------------------------------|
| <b>Models</b><br>EL-D<br>ELC-D<br>ELV-D<br>ELVC-D |    | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode | <b>Units</b><br>°C<br>Min | <b>Factory Setting</b><br>134<br>3<br>Fast          |
|                                                   |                                                                                     | <b>Notes:</b>                                                                                 |                           |                                                     |
| Program 2                                         |                                                                                     | Plastic (Fast Exhaust)                                                                        |                           |                                                     |
| <b>Models</b><br>EL-D<br>ELC-D<br>ELV-D<br>ELVC-D |    | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode | <b>Units</b><br>°C<br>Min | <b>Factory Setting</b><br>121<br>15<br>Fast         |
|                                                   |                                                                                     | <b>Notes:</b>                                                                                 |                           |                                                     |
| Program 3                                         |                                                                                     | Liquid A (Slow Exhaust)                                                                       |                           |                                                     |
| <b>Models</b><br>EL-D<br>ELC-D<br>ELV-D<br>ELVC-D |   | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>15<br>Slow         |
|                                                   |                                                                                     | <b>Notes:</b>                                                                                 |                           |                                                     |
| Program 4                                         |                                                                                     | Liquids B / Waste (Slow Exhaust)                                                              |                           |                                                     |
| <b>Models</b><br>EL-D<br>ELC-D<br>ELV-D<br>ELVC-D |  | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>30<br>Slow         |
|                                                   |                                                                                     | <b>Notes:</b>                                                                                 |                           |                                                     |
| Program 5                                         |                                                                                     | Liquid A – Fast Cooling                                                                       |                           |                                                     |
| <b>Models</b><br>ELC-D<br>ELVC-D                  |  | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>15<br>Fast Cooling |
|                                                   |                                                                                     | <b>Notes:</b>                                                                                 |                           |                                                     |
| Program 6                                         |                                                                                     | Liquid B – Fast Cooling                                                                       |                           |                                                     |
| <b>Models</b><br>ELC-D<br>ELVC-D                  |  | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>30<br>Fast Cooling |
|                                                   |                                                                                     | <b>Notes:</b>                                                                                 |                           |                                                     |

# TECHNICAL SPECIFICATION – LABORATORY Autoclaves

## Benchtop and Vertical Series

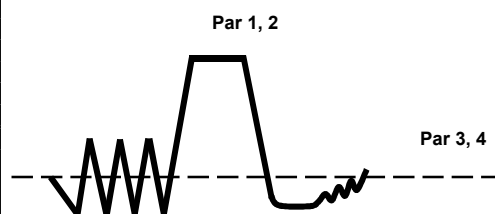
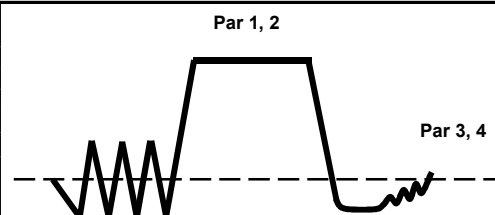
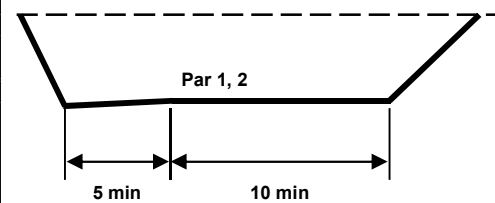

### PROGRAMS 7 TO 12

| Program 7                                                                                |                                                                                     | Glass                                                                                                                                                                                                                                                                         |                           |                                                     |
|------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------|-----------------------------------------------------|
| <b>Models</b><br>ELC-D-PV<br>ELVC-D-PV<br>ELC-D-PVG<br>ELVC-D-PVG                        |    | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode                                                                                                                                                                                 | <b>Units</b><br>°C<br>Min | <b>Factory Setting</b><br>134<br>3<br>Fast          |
|                                                                                          |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 1 vacuum pulses (down to 25 kPa). When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa.                                                                               |                           |                                                     |
| Program 8                                                                                |                                                                                     | Plastic                                                                                                                                                                                                                                                                       |                           |                                                     |
| <b>Models</b><br>EL-D-PV<br>ELV-D-PV<br>ELC-D-PV<br>ELVC-D-PV<br>ELC-D-PVG<br>ELVC-D-PVG |    | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode                                                                                                                                                                                 | <b>Units</b><br>°C<br>Min | <b>Factory Setting</b><br>121<br>15<br>Fast         |
|                                                                                          |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 1 vacuum pulses (down to 25 kPa). When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa.                                                                               |                           |                                                     |
| Program 9                                                                                |                                                                                     | Liquids A: slow exhaust                                                                                                                                                                                                                                                       |                           |                                                     |
| <b>Models</b><br>EL-D-PV<br>ELV-D-PV<br>ELC-D-PV<br>ELVC-D-PV<br>ELC-D-PVG<br>ELV-D-PVG  |   | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode                                                                                                                                                                                 | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>15<br>Slow         |
|                                                                                          |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 1 vacuum pulses (down to 25 kPa). When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa. Exhaust time is dependent on load volume and configuration of bottles/flasks. |                           |                                                     |
| Program 10                                                                               |                                                                                     | Liquids B: slow exhaust                                                                                                                                                                                                                                                       |                           |                                                     |
| <b>Models</b><br>EL-D-PV<br>ELV-D-PV<br>ELC-D-PV<br>ELVC-D-PV<br>ELC-D-PVG<br>ELV-D-PVG  |  | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode                                                                                                                                                                                 | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>30<br>Slow         |
|                                                                                          |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 1 vacuum pulses (down to 25 kPa). When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa. Exhaust time is dependent on load volume and configuration of bottles/flasks. |                           |                                                     |
| Program 11                                                                               |                                                                                     | Liquids A – Fast Cooling<br>Slow exhaust                                                                                                                                                                                                                                      |                           |                                                     |
| <b>Models</b><br>ELC-D-PV<br>ELVC-D-PV<br>ELC-D-PVG<br>ELVC-D-PVG                        |  | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode                                                                                                                                                                                 | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>15<br>Fast Cooling |
|                                                                                          |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 1 vacuum pulses (down to 25 kPa). When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa.                                                                               |                           |                                                     |
| Program 12                                                                               |                                                                                     | Liquids B – Fast Cooling<br>Slow exhaust                                                                                                                                                                                                                                      |                           |                                                     |
| <b>Models</b><br>ELC-D-PV<br>ELVC-D-PV<br>ELC-D-PVG<br>ELVC-D-PVG                        |  | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode                                                                                                                                                                                 | <b>Units</b><br>°C<br>min | <b>Factory Setting</b><br>121<br>30<br>Fast Cooling |
|                                                                                          |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 1 vacuum pulses (down to 25 kPa). When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa.                                                                               |                           |                                                     |

# TECHNICAL SPECIFICATION – LABORATORY Autoclaves

## Benchtop and Vertical Series

### PROGRAMS 13 TO 17

| Program 13                                                                                   |                                                                                     | Waste                                                                                                                                                                                                                                                                     |                                      |                                                   |
|----------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------|---------------------------------------------------|
| <b>Models</b><br><br>ELC-D-PVG<br>ELVC-D-PVG                                                 |    | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode<br>4. Drying Time (Post-Vacuum)                                                                                                                                             | <b>Units</b><br>°C<br>Min<br><br>min | <b>Factory Setting</b><br>134<br>7<br>Fast<br>15  |
|                                                                                              |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 4 vacuum pulses (down to 25 kPa) and 3 steam pulses up to 160 kPa. When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa. Exhausts effluents to Bio-Hazard system. |                                      |                                                   |
| Program 14                                                                                   |                                                                                     | Hollow Load                                                                                                                                                                                                                                                               |                                      |                                                   |
| <b>Models</b><br><br>ELC-D-PVG<br>ELVC-D-PVG                                                 |    | <b>Parameters</b><br>1. Sterilization Temperature<br>2. Sterilization Time<br>3. Exhaust Mode<br>4. Drying Time (Post-Vacuum)                                                                                                                                             | <b>Units</b><br>°C<br>min<br><br>min | <b>Factory Setting</b><br>121<br>15<br>Fast<br>15 |
|                                                                                              |                                                                                     | <b>Notes:</b><br>Residual air is displaced by 4 vacuum pulses (down to 25 kPa) and 3 steam pulses up to 160 kPa. When the pressure reaches atmospheric pressure the vacuum pump is activated until the pressure drops to 25 kPa.                                          |                                      |                                                   |
| Program 15                                                                                   |                                                                                     | Air Leakage/Vacuum Test                                                                                                                                                                                                                                                   |                                      |                                                   |
| <b>Models</b><br><br>EL-D-PV<br>ELV-D-PV<br>ELC-D-PV<br>ELVC-D-PV<br>ELC-D-PVG<br>ELVC-D-PVG |   | <b>Parameters</b><br>1. Stabilizing Time<br>2. Test Time                                                                                                                                                                                                                  | <b>Units</b><br>min<br>min           | <b>Factory Setting</b><br>5<br>10                 |
|                                                                                              |                                                                                     | <b>Notes:</b><br><br>Chamber vacuum is brought to 10 kPa. Thereafter all valves and motors are closed for 5 minutes enabling pressure stabilization.                                                                                                                      |                                      |                                                   |
| Program 16                                                                                   |                                                                                     | Isothermal                                                                                                                                                                                                                                                                |                                      |                                                   |
| <b>Optional for all Models</b>                                                               |  | <b>Parameters</b><br>1. Isothermal Temperature<br>2. Isothermal Time                                                                                                                                                                                                      | <b>Units</b><br>°C<br>min            | <b>Factory Setting</b><br>85<br>15                |
|                                                                                              |                                                                                     | <b>Notes:</b>                                                                                                                                                                                                                                                             |                                      |                                                   |
| Program 17                                                                                   |                                                                                     | Warm Up                                                                                                                                                                                                                                                                   |                                      |                                                   |
| <b>Optional for all Models</b>                                                               |  | <b>Parameters</b><br>1. Warm Up Temperature<br>2. Warm Up Time                                                                                                                                                                                                            | <b>Units</b><br>°C<br>min            | <b>Factory Setting</b><br>60<br>15                |
|                                                                                              |                                                                                     | <b>Notes:</b>                                                                                                                                                                                                                                                             |                                      |                                                   |

### SPECIAL OPTIONS AND ACCESSORIES

#### CONTROL SYSTEM OPTIONS

##### **Independent Temperature Probe (PT100)**

Independent probe that can be connected to an external independent device.

##### **External Independent Recorder**

This external recorder, with independent microprocessor control and power supply, is suitable for independent cycle documentation. This multi-range input recorder can record 4 channels at once from PT100s and/or pressure transducer. Simple operation with an easy-to-view display allows one to key-in various items of set data. The unit operates independently of the autoclave.

##### **Special Custom Cycles**

Other special programs like: glass-test, repeating program run, material stress test, Durham program, long term test (days long), aging test, varnish test, and other application related programs are optionally available.

#### SOFTWARE OPTIONS

##### **R.PC.R (Remote PC Reporting)**

PC software for generating reports which include:

- graph of the cycle data
- numeric data of the cycle
- copy of cycle print-outs
- table of all measured values
- table of all parameters
- option to save all reports in PDF file format

The software allows 2 modes of operation:

##### Online mode

Up to 8 autoclaves may be accessed using a PC within the organization via an Ethernet connection. These autoclaves can each be remotely monitored at the same time showing all reports and graphs. History files are automatically downloaded from the autoclave.

##### Offline mode

Data is transferred from the autoclave using a standard USB memory device. This data can then be viewed with the report generator software on a PC.

### CONTACT INFORMATION

#### **International Sales and Marketing**

E-mail: [info@tuttnauer-hq.com](mailto:info@tuttnauer-hq.com)

Website: [www.tuttnauer.com](http://www.tuttnauer.com)

#### **Tuttnauer Europe b.v.**

Hoeksteen 11, 4815 PR

P.O.B. 7191, 4800 GD Breda

The Netherlands

Tel: +31 (0) 765 423 510 Fax: +31 (0) 765 423 540

E-mail: [info@tuttnauer.nl](mailto:info@tuttnauer.nl)

#### HARDWARE OPTIONS

Note: Other hardware options such as vacuum pump, steam generator, etc. have been mentioned above in relevant sections.

##### **Air Compressor**

Introduces pressurized air into the chamber for rapid cooling of liquids for models with a fast cooling system.

Not needed if air pressure source is available on site.

##### **Printer**

Internal thermal printer for cycle documentation. During the cycle the printer records temperature, pressure, time, date, cycle status, end of cycle.

##### **IQ, OQ, PQ**

Installation Qualification (IQ) - documentary evidence to verify that the equipment has been built and installed in compliance with design specifications.

Operational Qualification (OQ) Preliminary Operational Qualification (OQ) - documentary evidence to verify that the equipment operates in accordance with its design specifications in its normal operating range and performs as intended throughout all anticipated operating ranges.

Preliminary Performance Qualification (PQ) - documentary evidence which verifies that the equipment or system operates consistently and gives reproducibility within defined specifications and parameters for prolonged periods.

##### **Switch Box**

Switch box from 3-phases to 1-phase, requested current 40A.

##### **Mobile Lifting Device**

The mobile lifting device for vertical autoclave basket with heavy sterilisation load up to 150 kg. The lift is mobile equipped with an integrated swivel arm for maximum maneuverability and can service a few autoclaves. Controlled by push buttons on a movable control handset. Equipped with a maintenance free electrical battery

##### **Loading Equipment**

Loading carts and transfer carriages on rails to assist the loading and unloading process. Constructed of high quality, durable stainless steel. The adjustable loading cart rolls from the transfer carriage onto the interior chamber tracks for easy handling of heavy loads.

