



HALO[®]

PCS


POSITIVELY EXCEPTIONAL PERFORMANCE



HALO[®] PCS C18

POSITIVE RESULTS FOR BASIC COMPOUNDS

Built upon proven Fused-Core[®] technology for speed and efficiency, the HALO[®] PCS C18 is a positively charged surface chemistry designed to deliver improved peak shapes for basic compounds. Ideal for use with low ionic strength mobile phases, HALO[®] PCS maintains peak symmetry at higher loading capacities and provides an alternate selectivity from other C18 bonded phases. Available in both a 90 Å and 160 Å pore size for small molecule and peptide analysis.

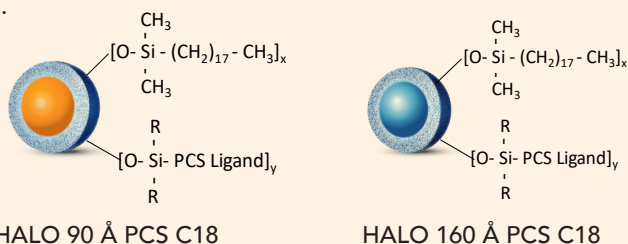

FEATURES OF HALO[®] PCS C18


- Excellent peak shape and increased loading capacity for basic compounds
- Lot-to-Lot reproducibility
- UHPLC and LCMS compatible
- Alternate L1 selectivity
- Built upon Fused-Core[®] technology for fast, efficient and reliable separations

Best Applications:

- Reversed-phase separations of basic analytes prone to peak tailing
- Peptide mapping
- Basic pharmaceutical compounds

QUALITY YOU CAN COUNT ON

Panel of antidepressants screened over 1000 injections (10,000 column volumes) demonstrates the excellent stability of HALO[®] PCS C18.

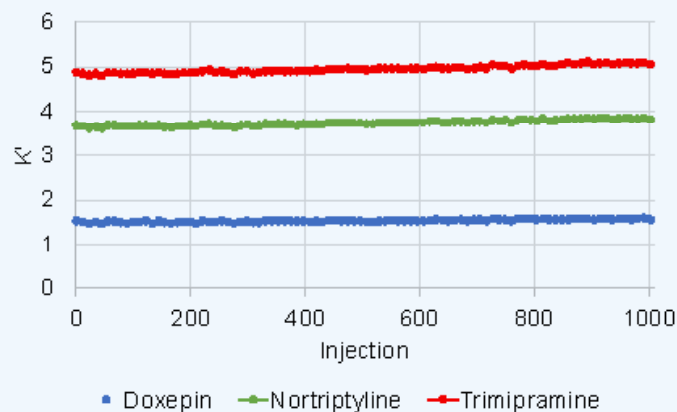


TEST CONDITIONS:

Column: HALO 90 Å PCS C18, 2.7 μm, 2.1 x 100 mm
 Part Number: 77148-028
 Mobile Phase:
 A: Water, 0.1% Formic Acid
 B: Acetonitrile, 0.1% Formic Acid
 Isocratic: 20% B
 Flow Rate: 0.6 mL/min
 Back Pressure: 244 bar

Temperature: 60 °C
 Injection: 0.5 μL
 Sample Solvent: 80/20 Water/ ACN
 Wavelength: PDA, 254 nm
 Flow Cell: 1 μL
 Data Rate: 40 Hz
 Response Time: 0.025 sec.
 LC System: Shimadzu Nexera X2

Lot to Lot comparison demonstrates reproducibility and good peak shapes for basic, acidic and neutral compounds.

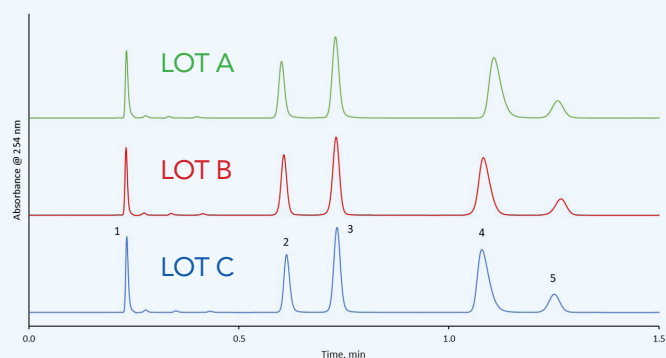

PEAK IDENTITIES:

- | | |
|--------------------------|-----------------------|
| 1. Uracil | 4. Imipramine |
| 2. 2-Chlorobenzoic Acid | 5. Dimethyl Phthalate |
| 3. 4-Methoxybenzoic Acid | |

TEST CONDITIONS:


Column: HALO 90 Å PCS C18, 2.7 μm, 4.6 x 50 mm
 Part Number: 77148-042
 Mobile Phase:
 A: 15 mM Ammonium Formate, 0.1% Formic Acid
 B: Acetonitrile, 0.1% Formic Acid
 Isocratic: 30% B
 Flow Rate: 1.8 mL/min

Back Pressure: 225 bar
 Temperature: 35 °C
 Injection: 1.0 μL
 Sample Solvent: 70/30 Water/ ACN
 Wavelength: PDA, 254 nm
 Flow Cell: 1 μL
 Data Rate: 40 Hz
 Response Time: 0.025 sec.
 LC System: Shimadzu Nexera X2

APPLICATIONS

BETA BLOCKERS SEPARATION ON HALO® PCS C18

Eleven different beta blockers are separated in under 5 minutes using the HALO® PCS C18 column and demonstrating the speed and resolution of Fused-Core® technology.

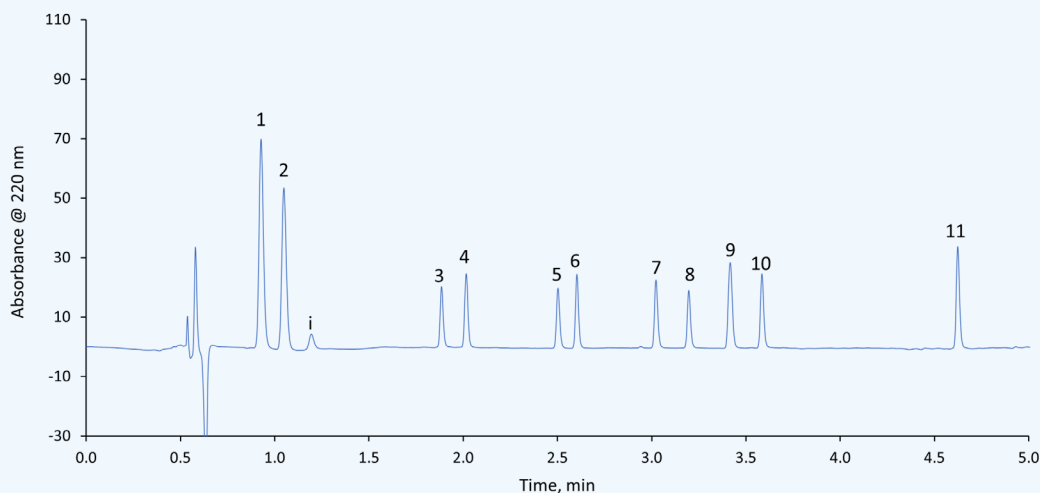

PEAK IDENTITIES:

1. Sotalol
2. Atenolol
3. Pindolol
4. Nadolol
5. Metoprolol
6. Acebutolol
7. Oxprenolol
8. Bisoprolol
9. Labetalol
10. Propranolol
11. Carvedilol

i = impurity in bisoprolol

TEST CONDITIONS:

Column: HALO 90 Å PCS C18, 2.7 µm, 2.1 x 100 mm
Part Number: 77148-028
Mobile Phase:
A: Water, 0.1% Formic Acid
B: Acetonitrile, 0.1% Formic Acid

Gradient Separation:


Time:	%B
0.00	3
5.00	36
6.50	100
7.50	100
8.00	3
12.00	3

Flow Rate: 0.4 mL/min
Back Pressure: 281 bar
Temperature: 30°C
Injection: 1.0 µL
Sample Solvent: 93/7 Water/ACN
Wavelength: PDA, 220 nm
Flow Cell: 1 µL

Data Rate: 100 Hz
Response Time: 0.025 sec.
LC System: Shimadzu Nexera X2

FUSED-CORE® ADVANTAGE

As shown in this basic drug panel of antidepressants, the HALO® Fused-Core® PCS technology tolerates a higher sample load of basic compounds compared to the competitor fully porous C18 column. The positive charged surface (PCS) stationary phase is ideal for basic analytes when using low ionic strength mobile phases such as formic acid.

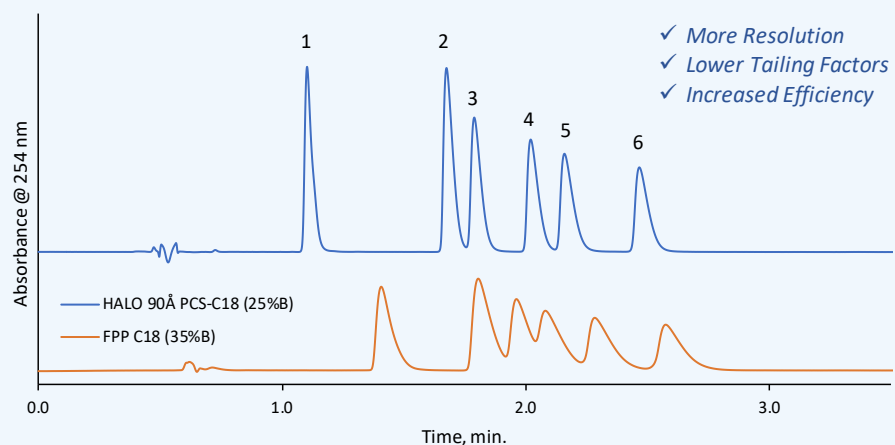

- ✓ More Resolution
- ✓ Lower Tailing Factors
- ✓ Increased Efficiency

TEST CONDITIONS:

Column: HALO 90 Å PCS C18, 2.7 µm, 2.1 x 100 mm
Part Number: 77148-028
Competitor Column: FPP C18, 3 µm, 2.1 x 100 mm
Mobile Phase A: Water, 0.1% Formic Acid
Mobile Phase B: Acetonitrile, 0.1% Formic Acid
Isocratic: HALO® PCS C18: 25% B
FPP C18: 35% B

Flow Rate: 0.4 mL/min
Back Pressure: 267 bar
Temperature: 35 °C
Injection: 0.5 µL (40 µg)
Sample Solvent: 75/25 Water/ ACN
Wavelength: PDA, 254 nm
Flow Cell: 1 µL
Data Rate: 100 Hz
Response Time: 0.025 sec.
LC System: Shimadzu Nexera X2


PEAK IDENTITIES:

1. Doxepin
2. Desipramine
3. Imipramine
4. Nortriptyline
5. Amitriptyline
6. Trimipramine

APPLICATIONS

SPP CHARGED SURFACE COMPARISON

In a head to head comparison of SPP columns, HALO[®] PCS C18 delivers better resolution, improved tailing factors and more plates over the leading competitor.

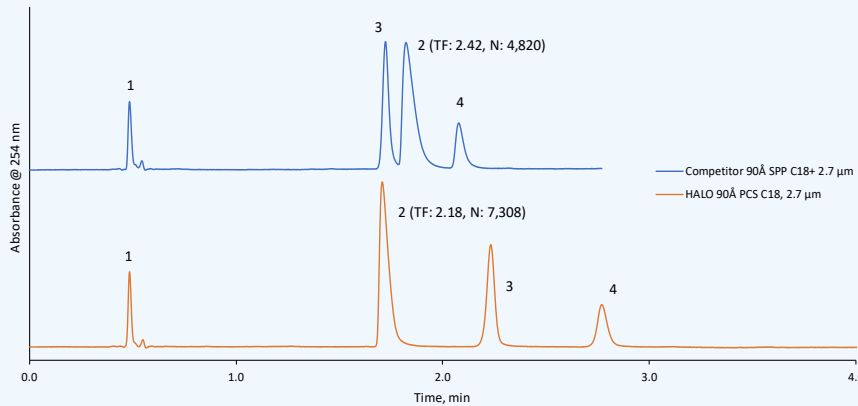

TEST CONDITIONS:


Column: HALO 90 Å PCS C18, 2.7 μm, 2.1 x 100 mm
Part Number: 77148-028
Mobile Phase:
A: Water, 0.1% Formic Acid
B: Acetonitrile, 0.1% Formic Acid
Isocratic: HALO[®] PCS C18: 24% B
Competitor C18+: 26% B
Flow Rate: 0.4 mL/min
Back Pressure: 238 bar
Temperature: 35 °C
Injection: 0.5 μL
Sample Solvent: 70/30 Water/ ACN
Wavelength: PDA, 254 nm
Flow Cell: 1 μL
Data Rate: 100 Hz
Response Time: 0.025 sec.
LC System: Shimadzu Nexera X2

PEAK IDENTITIES:

1. Uracil
2. Imipramine
3. 4-Methoxybenzoic Acid
4. 2-Chlorobenzoic Acid

PEPTIDE LOADING STUDIES

A HALO 160 Å PCS C18 column outperforms a traditional C18 column under formic acid conditions due to its positive charge surface, allowing for improved peak shape and resolution for peptides. PCS C18 also allows for a higher sample load on column for basic analytes and could potentially help pull apart closely retained impurities as seen below.

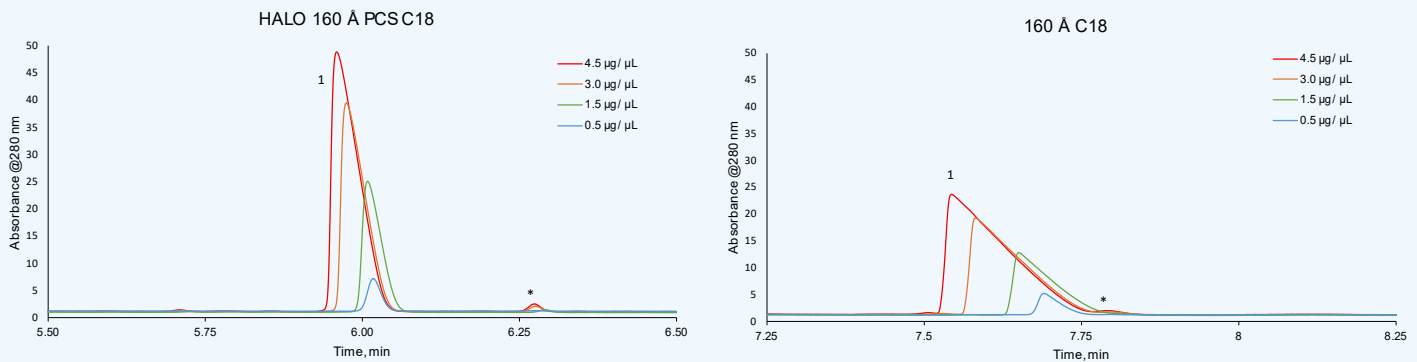

PEAK IDENTITIES:

1. 5Y Sequence: Ac-RGVVGLYLKG-NH₂ (1102 Da)
- * Impurity

TEST CONDITIONS:

Column: HALO 160 Å PCS-C18, 2.7 μm, 4.6 x 100 mm
Part Number: 77148-014
Mobile Phase A: Water/ 0.1% Formic Acid
Mobile Phase B: Acetonitrile/ 0.1% Formic Acid
Gradient:


Time	% B
0.0	0
10.0	35

Flow Rate: 1.5 mL/min
Pressure: 309 bar
Temperature: 30 °C
Injection Volume: 1, 5, 10, 15 μL (0.3 μg/μL)
Wavelength: PDA, 280 nm
Flow Cell: 1 μL
Data Rate: 100 Hz
Response Time: 0.025 sec.
LC System: Shimadzu Nexera X2

APPLICATIONS

HALO 160 Å PCS C18 RAPID PEPTIDE SEPARATION

A separation of peptides is performed on a HALO 160 Å PCS C18 column showing excellent peak shape under formic acid conditions. With Fused-Core® technology flow rates are able to be increased while maintaining column efficiencies allowing for fast, high throughput separations.

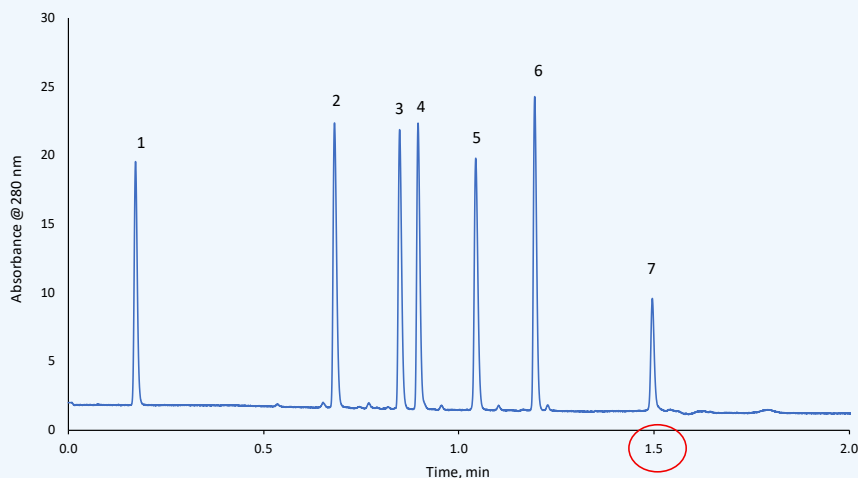

TEST CONDITIONS:


Column: HALO 160 Å PCS C18 , 2.7 µm, 2.1 x 50 mm
Part Number: 77147-996
Mobile Phase A: Water/ 0.1% Formic Acid
Mobile Phase B: Acetonitrile/ 0.1% Formic Acid
Gradient: Time % B
0.0 0
1.5 35
2.0 35
Flow Rate: 1.0 mL/min
Pressure: 360 bar
Temperature: 30 °C
Injection Volume: 1.0 µL (0.3 µg/µL)
Wavelength: PDA, 280 nm
Flow Cell: 1 µL
Data Rate: 100 Hz
Response Time: 0.025 sec.
LC System: Shimadzu Nexera X2

PEAK IDENTITIES:

- | | |
|-------------------------------------|-------------------------------------|
| 1. Uracil | 5. S4Y2 Sequence: Ac-RGVGYLGLGK-NH2 |
| 2. S1Y Sequence: RGAGGLYL GK-NH2 | 6. S5Y Sequence: Ac-RGVVGLYL GK-NH2 |
| 3. S2Y Sequence: Ac-RGGGGLYL GK-NH2 | 7. Insulin Chain B Oxidized |
| 4. S3Y Sequence: Ac-RGAGGLYL GK-NH2 | |

THE PCS ADVANTAGE

A synthetic panel of basic peptides is screened on the HALO 160 Å PCS C18 compared to the traditional C18 stationary phase. While using low ionic strength mobile phases such as formic acid the positively charged surface stationary phase shows significantly better peak widths and symmetry for more basic peptides when compared to a traditional non-encapped peptide C18 stationary phase.

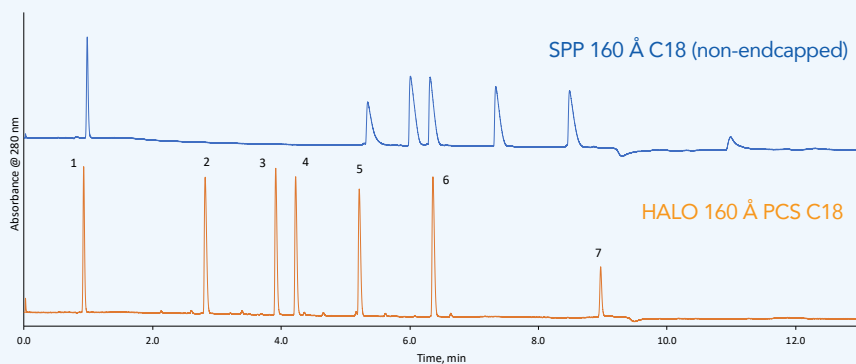

TEST CONDITIONS:

Column: HALO 160 Å PCS C18 , 2.7 µm, 2.1 x 100 mm
Part Number: 77147-998
Comparison Column: SPP 160 Å C18, 2.7 µm, 2.1 x 100mm
Mobile Phase A: Water/ 0.1% Formic Acid
Mobile Phase B: Acetonitrile/ 0.1% Formic Acid
Gradient: Time % B
0.0 2
10.0 35
Flow Rate: 0.3 mL/min
Temperature: 30 °C
Injection Volume: 1.0 µL
Wavelength: PDA, 280 nm
Flow Cell: 1 µL
Data Rate: 100 Hz
Response Time: 0.025 sec.
LC System: Shimadzu Nexera X2

PEAK IDENTITIES:

- | | |
|-------------------------------------|-------------------------------------|
| 1. Uracil | 5. S4Y2 Sequence: Ac-RGVGYLGLGK-NH2 |
| 2. S1Y Sequence: RGAGGLYL GK-NH2 | 6. S5Y Sequence: Ac-RGVVGLYL GK-NH2 |
| 3. S2Y Sequence: Ac-RGGGGLYL GK-NH2 | 7. Insulin Chain B Oxidized |
| 4. S3Y Sequence: Ac-RGAGGLYL GK-NH2 | |

SPECIFICATIONS

Ligand: dimethyloctadecylsilane
 Particle Size: 2.7 μm
 Pore Size: 90 and 160 \AA
 USP Designation: L1

Carbon Load 90 \AA : 7.5%
 Carbon Load 160 \AA : 5.09%
 Surface Area 90 \AA : 135 m^2/g
 Surface Area 160 \AA : 90 m^2/g

Endcapped: Yes both 90 and 160 \AA
 Low pH Limit /Max T: 2/60 $^{\circ}\text{C}$
 High pH Limit/Max T: 7/40 $^{\circ}\text{C}$

PART NUMBERS

HALO 90 \AA PCS C18 SMALL MOLECULE COLUMNS	
Dimensions: ID x Length (in mm)	Part Number
1.5 x 50	77148-050
1.5 x 100	77148-052
1.5 x 150	77148-054
2.1 x 50	77148-026
2.1 x 100	77148-028
2.1 x 150	77148-030
3.0 x 50	77148-034
3.0 x 100	77148-036
3.0 x 150	77148-038
4.6 x 50	77148-042
4.6 x 100	77148-044
4.6 x 150	77148-046
4.6 x 250	77148-048

HALO 160 \AA PCS C18 PEPTIDE COLUMNS	
Dimensions: ID x Length (in mm)	Part Number
1.5 x 50	77148-018
1.5 x 100	77148-020
1.5 x 150	77148-022
2.1 x 50	77147-996
2.1 x 100	77147-998
2.1 x 150	77148-000
3.0 x 50	77148-004
3.0 x 100	77148-006
3.0 x 150	77148-008
4.6 x 50	77148-012
4.6 x 100	77148-014
4.6 x 150	77148-016

HALO 90 \AA PCS C18 GUARD COLUMNS	
Guard columns, 3-pack	
Dimensions: ID x Length (in mm)	Part Number
2.1 x 5	77148-024
3.0 x 5	77148-032
4.6 x 5	77148-040
Guard Column Holder	76445-284


HALO 160 \AA PCS C18 GUARD COLUMNS	
Guard columns, 3-pack	
Dimensions: ID x Length (in mm)	Part Number
2.1 x 5	77147-994
3.0 x 5	77148-002
4.6 x 5	77148-010
Guard Column Holder	76445-284

INNOVATION YOU CAN TRUST – PERFORMANCE YOU CAN RELY ON

HALO and Fused-Core are registered trademarks of Advanced Materials Technology, Inc.

Advanced Materials Technology is an ISO 9001:2015 Certified Company

HALO®

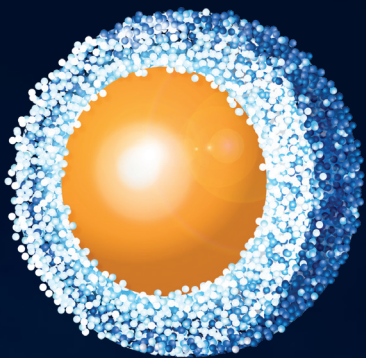

Manufactured by:



advancedmaterialstechnology

 **avantor™**
delivered by **VWR™**

VWR.COM

Prices, product, and/or services details are current when published and subject to change without notice. | Certain products or services may be limited by federal, state, provincial, or local regulations. | VWR, part of Avantor, makes no claims or warranties concerning sustainable/green products. Any claims concerning sustainable/green products are the sole claims of the manufacturer and not those of VWR International, LLC and/or Avantor, Inc. or affiliates. All prices are in US dollars unless otherwise noted. Offers valid in US and Canada unless otherwise noted, void where prohibited by law or company policy, while supplies last. | Trademarks are owned by Avantor, Inc. or its affiliates, unless otherwise noted. | Visit vwr.com to view our privacy policy, trademark owners, and additional disclaimers. © 2023 Avantor, Inc. All rights reserved.